

id100-20 Single Photon Detection Module

Application Note: Fluorescence Lifetime Measurement

We thank you for your interest in our products. This application note explains the advantages brought by the id100-20 module (see Fig.1) over commercially available photomultiplier tubes (PMTs) and single photon counting modules for fluorescence lifetime measurements.

Fluorescence lifetime measurements based on near field or confocal microscopy find applications in various fields such as biochemistry and analytical chemistry, medicine, pharmacology, photophysics and photochemistry, and environmental research. Over the past few years we have witnessed a tremendous surge of interest in single molecule detection (SMD) by Time Correlated Single Photon Counting technique (TCSPC). In single molecule detection applications, the molecules to be detected are fluorescently labelled. By repetitive laser excitations, the fluorescent molecule is cycled between its ground state and the excited state. The excited state exists for a finite time, i.e. the fluorescence lifetime during which the energy is partially dissipated until the relaxed singlet excited state is reached. Then, the fluorophore returns to its ground state by fluorescence, i.e. by emission of a photon of wavelength λ_{fluor} . After many excitation pulses, the fluorescence lifetime, i.e. the average time the fluorophore spends in the excited state, is obtained, allowing the identification of the molecule.

A typical set-up (see Fig.2) for fluorescence decay time measurement includes a pulsed laser diode, appropriate lenses for beam expansion, a microscope objective to focus the excitation beam and collect the emitted fluorescence photons, a set of appropriate lenses to focus the light on the id100-20 photosensitive area and a bandpass filter centered on λ_{fluor} . A time-to-digital converter (TDC) or time-to-amplitude converter combined with a multichannel analyzer measures the time between the laser excitation and the fluorescent photon emission. A histogram is progressively built and the fluorescent decay time is extracted.

For your fluorescence lifetime measurements, the id100-20 offers:

☞ **a best-in-class timing resolution of 40ps FWHM** (see Fig.3). This is a significant improvement compared to photomultiplier tubes and other commercially available photon counting modules. This excellent feature allows accurate measurements of extremely short fluorescence lifetimes of a few tens of picoseconds. Furthermore, multi-component fluorescence decay time experiments become possible with high resolution.

☞ **a large range of sensitivity**. With a maximum in the green and a single photon sensitivity covering the entire visible range (400 to 750nm), *id Quantique's* id100-20 is suited for most fluorophores used in life sciences (see <http://microscopy.bio-rad.com/fluorescence/fluorophoradata.htm>). The id100-20 photon detection probability compares favorably with standard PMTs.

☞ **a dead time of 70ns**, which allows a maximum excitation frequency of 14MHz. The histogram can thus be recovered in a very short time.

☞ **a low rate of spurious counts** including afterpulses and dark counts that usually damage the signal-to-noise ratio of your measurement. The low dark count and afterpulsing rates are obtained by limiting the active area diameter to 20 μ m. A carefully studied optical set-up is thus required to focus the fluorescence light onto the detector active area. *id Quantique* recommends to mount the id100-20 on a 3-axis translation stage using the available mounting brackets. A precise alignment is thus possible and only needs to be done once. Due to the limited detector area, the presence of a pinhole in front of the detector is often unnecessary. *id Quantique* also offers a fiber-coupled version of the id100-20 with a 50 μ m-core multimode fiber.

☞ **a compact design** and a high level of reliability. In addition, the id100-20 is **not damaged by ambient light** and is **immediately operational** as no cooling is required.

For **parallel measurements**, *id Quantique* has introduced the id150. This **1x10 linear array of single photon detectors** is the first commercially available product allowing high throughput parallel photon counting and timing measurements (<http://www.idquantique.com/spcm-vis-10.html>). For further information on our products, please contact *id Quantique* by phone: +41 (0)22 301 83 71, fax: +41 (0)22 301 83 79, or email: sales@idquantique.com. Note that *id Quantique* also offers photon counting modules operating in the infrared and short-pulse laser sources. Custom developments of single photon sensors including arrays are possible.



Fig. 1: Photomicrograph of the *id Quantique's* id100-20.

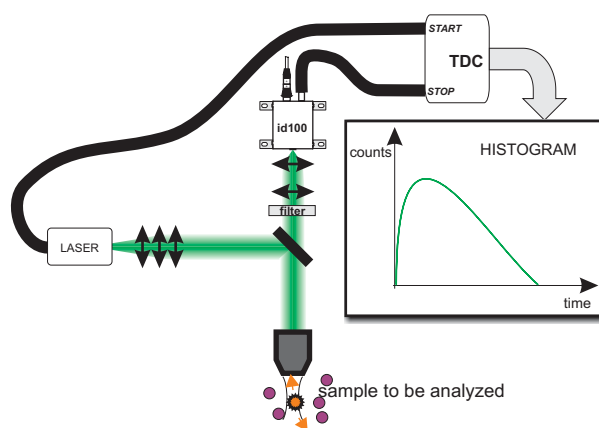


Fig. 2: Typical set-up for fluorescence lifetime measurement.

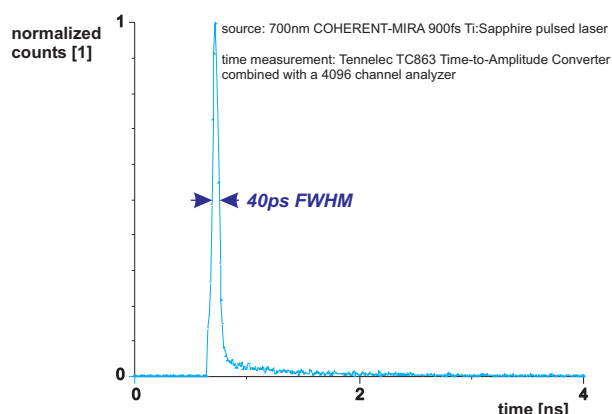


Fig. 3: Timing resolution of the *id Quantique's* id100-20.



光技術をサポートする
株式会社オプトサイエンス
<http://www.optoscience.com>

東京本社 〒160-0014 東京都新宿区内藤町1番地 内藤町ビルディング
TEL:03(3356)1064 FAX:03(3356)3466 E-mail: info@optoscience.com
大阪支店 〒532-0011 大阪市淀川区西中島7-7-2 新大阪ビル西館
TEL:06(6305)2064 FAX:06(6305)1030 E-mail: osk@optoscience.com
名古屋営業所 〒450-0002 名古屋市中村区名駅2-37-21 東海ソフトビル
TEL:052(569)6064 FAX:052(569)8064 E-mail: ngo@optoscience.com

id Quantique